Table of Contents

SAFETY INS	STRUCTION	3
OVERVIEW	Safety Symbols	5
	Models Introduction.5Main Characteristics.5Rear Panel Overview.6	
FRONT PAN	IEL INTRODUCTION	6
	Panel Overview6Display6Status Indication6Storage Indication7Brief Introduction of Panel Buttons7	
REAR PAN	ELINTRODUCTION	9
OPERATIO	N	0
	Power Up. 10 Output ON/OFF. 11 Beep ON/OFF. 11 Panel Lock. 11 Output Parameters Setup 12 Save Setup 12 Recall Setup 13	

REMOTE CONTROL1	44
Remote Control Setup 14	
Remote control procedures 15	
FAQ1	616
SPECIFICATIONS 1	17

The proprietary information in this manual is protected by copyrights. Any photocopies, reproductions or translation to another language are not allowed unless it is permitted by KORAD Technology officially. And all rights are reserved.

The information in this manual is correct when printing. However, KORAD will continuously improve products and reserve the rights to change specifications, equipment, and maintenance procedures at any time without notice.

SHENZHEN KORAD TECHNOLOGY CO. LTD.

Reaction Time Volta ge Rise Volta ge Drop ≤100mS ≤100mS

Interface

Optional Interfaces (for program mable models only): RS232, USB

Accessories

User manual *1, ; Power cord*1

Weight and Dimension

 $110 mm(W)^*156 mm(H)^*260(D)KA3003x3.6Kg, KA3005, KA6002x4.8Kg, KA6005x7.5Kg, KA3010x7.5Kg$

SAFETY SYMBOLS

This chapter contains important safety instructions that you must follow when operating the KA3000 & KA6000 series and when keeping it in storage. Read the following before any operation to insure your safety and to keep the best condition for the KA3000 & KA6000 series.

Safety Symbols

These safety symbols may appear in this manual or on the series..



WARNING



DANGER High Voltage.



Earth (ground) Terminal

3

18

SAFETY INSTRUCTION

Safety Guidelines

- •Do not block or obstruct the cooling fan vent opening.
- •Avoid severe impacts or rough handling that leads to damage.
- •Do not discharge static electricity.
- •Do not disassemble unless you are qualified as service personnel.

AC INPUT



- •AC Inut Voltage: 110V / 120V / 220V / 230V , 50 / 60 Hz
- •Connect the protective grounding conductor of the AC power cord to an earth ground, to avoid electrical shock.

Operation Environment

•Location: Indoor, no direct sunlight, dust free, almost non-conductive pollution (note below)

•Relative Humidity: < 80%

•Altitude: < 2000m

•Temperature: 32 - 104°F

Storage environment

•Location: Indoor

•Relative Humidity: < 70% •Temperature:-10-70°C

FUSE

Model	110/120 VV	220/230 V	
KA3003D/P	T4A/ 250 V	T2A/250 V	
KA3005D/P	T5A/250V	T3A/250 V	
KA3010D/P	T10A/250V	T5A/250 V	
KA6003D/P	T5A/250 V	T3A/250 V	
KA 600 5D/P	T10A/ 250 V	T5A/250 V	

- •To ensure fire protection, replace the fuse only with the specified type and rating.
- •Disconnect the power cord before fuse replacement.
- •Make sure the cause of fuse blowout is fixed before fuse replacement.

KORAD

Specifications

Note: The specifications below are tested under the conditions of temperation 25%+-5% and the warm-up for 20 minutes.

	1/40000				
Models	KA3003	KA3005	KA3010	KA6003	KA6005
Voltage Range	0-30V	0-30V	0-30V	0-60V	0-60V
Current Range	0-3A	0-5A	0-10A	0-3A	0-5A
Load Re	gulation				
Current	≤0. 1%+5mA		≤0. 01%+3mv ≤0. 1%+20mA		≤0. 01%+2mv ≤0. 1%+10mA
Line Re	gulation				
Voltage Current	≤0. 01%+3mv ≤0. 1%+3mA	≤0. 01%+3mv ≤0. 1%+3mA		≤0. 01%+3mv ≤0. 1%+3mA	
Setup R	esolution				
Voltage Current		10m V 1 m A	10m V 1 m A	10m V 1 mA	10m V 1 m A
Setup A	ccuracy (25	°C+-5°C)			
Voltage Current	≤0.5%+20mV ≤0.5%+5mA	≤0.5%+20m V ≤0.5%+10m A	≤0.5%+20m V ≤0.5%+20m A		≤0.5%+30m V ≤0.5%+10m A
Ripple(2	20-20M)				
Voltage Current	≤1mVrms ≤3mArms	≤2mVrms ≤3mArms	≤2mVrms ≤5mArms	≤1m∨rms ≤3mArms	≤1m∨rms ≤3mArms
	oefficient				
Voltage Current	≤150ppm ≤150ppm	≤150ppm ≤150ppm	≤150ppm ≤150ppm	≤150ppm ≤150ppm	≤150ppm ≤150ppm
Read Ba	ack Resolution	n			
Voltage Current	10mV 1mA	10 m V 1 m A	10 m V 1 m A	10mV 1mA	10 mV 1 mA
Read Ba	ack Temp. Co	efficient			
Voltage Current	≤150 ppm ≤150ppm	≤150 ppm ≤150 ppm	≤150 ppm ≤150 ppm	≤150 ppm ≤150ppm	≤150 ppm ≤150ppm

FAQ

Q1: The panel buttons don't work when power on.

A1: The panel is locked. Press the button $\frac{LOCK}{UNICOCK}$ for over 2 seconds, and then the panel will unlock.

Q2: Pressing ON/OFF, there is no output when power on.

A2: Current setup is 0.

Q3: Output voltage rises slowly when output button is on.

A3: Current setup is too small.

Q4: Making OCP on and pressing output switch; and then the output is automatically shut off.

A4: Current protection value setup is too small. You could press output switch and then make OCP on.

Series Lineup/Main Features

		•			
	Model	V Meter	AMeter	USB	Resolution
_	KA3003D	4digit	4digit	NO	10mV/1mA
	KA3003P	4digit	4digit	Yes	10mV/1mA
	KA3005D	4digit	4digit	NO	10mV/1mA
_	KA3005P	4digit	4digit	Yes	10mV/1mA
_	KA3010D	4digit	4digit	NO	10mV/1mA
	KA3010P	4digit	4digit	Yes	10mV/1mA
	KA6003D	4digit	4digit	NO	10mV/1mA
	KA6003P	4digit	4digit	Yes	10mV/1mA
_	KA6005D	4digit	4digit	NO	10mV/1mA
_	KA6005P	4digit	4digit	Yes	10mV/1mA

Main Features

Performance

Operation


- Low noise: cooling fan controlled by Heatsink temperature;
- •
- Compact size, light weight.
 - Constant voltage / constant
 - Current operation
 - Output On / Off Control
 - Digital panel control
 - 4 pairs of panel setup save / recall
 - Coarse and fine Voltage / Current Control
 - Software calibration
 - Beep output
 - button lock function
 - Overload protection
 - Reverse polarity protection

Interfaces

Protection

 USB/RS232 for remote control(only For KA3003P,KA3005P,KA6003P)

Front Panel Overview

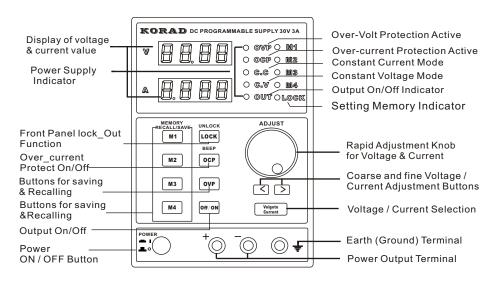

DISPLAY

Voltage level v



Voltmeter displays the setup value of output voltage .

Current level A



Displays the setup value of output current .

Condition Indication

OVP

OVP is the indicator of overvoltage protection. When overvoltage function is turned on, • • • Indicator lights on; when output voltage is higher than protection setup value due to unexpected conditions, output cuts off and OVP indicator flickers; Press the button OVP again, and the power supply recovers.

6

REMOTE CONTROL PROCEDURES

Entering the Remote Control Mode

- 1. Connect the USB cable.
- 2. The power supply will automatically connect. After normal connection, there will be a tweet from the power supply itself.
- 3. The panel buttons are locked, so the power supply can only controlled by the computer .

NOTE: KORAD software must be installed first.

Exiting from the Remote Control Mode

- 1. Close the remote control software.
- 2. Disconnect USB from the back.
- 3. The power supply disconnects; a tweet from the beep with the hint that the remote control is over.
- 4. The power supply automatically comes into the panel control mode.

15

REMOTE CONTROL

Remote Control Setup

All the models with the suffix "P", such as KA3003P, KA3005P, KA6002P, etc. can be connected to the PC through interfaces USB/RS232 on the back of the machine and controlled by the remote control.

COM setting

Set up the COM port inside the PC according to the following list.

Baud rate: 9600Parity bit: None

• Data bit: 8

• Stop bit: 1

· Data flow control: None

Functionality check

Run this query command via the terminal application such as MTTTY (Multi-threaded TTY). *DIN?

This should return the identification information: Manufacturer, model name, software version. KORAD KA3003P Vx.xx

KORAD

● ○©P OCP is OCP indicator. When overcurrent function is turned on, ○ ◎©P indicator lights on.

● ⑤□⑥ C.C is constant current indicator. When power supply is in the mode of constant current, this light is on.

● ©.▼ C.V is constant voltage indicator. When power supply is in the mode of constant voltage, this light is on.

• OUT is output indicator. If light on, there is voltage output in the output terminal.

Storage Indication

M1

M2
 Indication of saving and recalling 4 setups stored internally;

• M3 When LOCK indication turns on, the front panel button

M4 operation is locked.

● L@GK

Brief Introduction of Panel Operation



Saves or recalls panel settings. For settings, 1 ~ 4 are available. For save / recall details, see Page 13.

Recall Setup

The front panel settings can be recalled from one of the four internal memories.

M1 M2 M3


M4


Recalls panel settings. For settings, 1 ~ 4 are avai lable.

 \bigcirc M11 Indication of saving and recalling 4 setups stored O M2 internally; O M3 Press one of the 1 ~ 4 Memory buttons, for example number 1. The panel settings saved in memory \bigcirc M4

No. 1 are recalled. The LED M1 turns on.

When a setting is recalled, the output automatically Note: turns off.

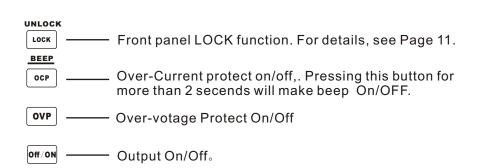



Voltage-Current Setting Adjustment

Digit Selector Buttons

Selection Voltage / Current for Adjustment Pressing the button, the volt indicator starts to blink; pressing it again, the ampere indicator starts to blink. Then turn the ADJUST knob and the settings of voltage or current can be adjusted.

POWER

On / Off main power. For power up sequence, see Page 10.



outputs voltage and current.



Connects the ground (earth) terminal.

Output Set

Panel operation

- 1. Connecting the load to the front port, red(+), black(-).
- 2. Setting output voltage and current.

 Press the button Voltage/Current selection to switch voltage adjustment and current adjustment. Adjusting voltage and current with Voltage / Current Adjustment knob. By default, the Voltage and Current knob work in the coarse mode. To activate the fine mode, press the buttons to select the coarse
- 3. Turning on the output and pressing the output button.
 The button LED turns on and displays CV or CC mode.

SAVE / RECALL SETUP

mode or the fine mode.

Save Setup

Background

The front panel settings can be stored into one of the four internal memories.

Contents

The following list shows the setup contents..


- •Fine / coarse knob editing mode
- ●Beep on / off
- •Output voltage / current level

The following settings are always saved as "off".

- ●Output on / off
- •Front panel lock on / off

Panel operation

Press one of the 4 buttons(M1,M2,M3,M4) and the LED light turns on accordingly. After you adjust the value, it is saved automatically once it stops blinking.

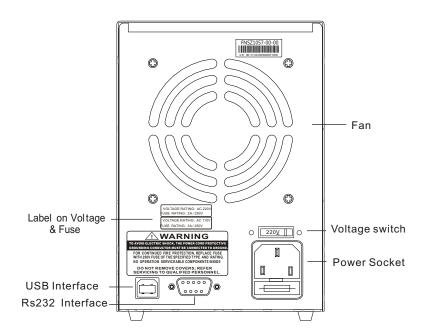



KORAD

RS232 dependent interface based on remote control order (see Page 14); only for KAXXXXP series, such as KA3003 P and so on.



RS232 dependent interface based on remote control order (see Page 14); only for KAXXXXP series, such as KA3003P and so on.



The power cord socket mainly accepts AC values: 115V / 230V, 50 / 60 Hz. Please refer to the fuse parameters on the back fuse label to replace the specified fuse.



Make sure the correct type of fuse is installed before power up

OPERATION

Connect AC power cord



Connecting AC power cord and selecting the corresponding AC voltage according to the back label on voltage; then connecting the AC power cord to the socket on the back panel

poweron



Press the power switch to turn power on. The display initializes, showing the model of the machine and then showing the setting last.

POWER

power off



Press the power switch again to turn power off.

10

Output On / Off

KORAD

Panel Operation

Press the Output button to turn on output; and the button LED also turns on. Pressing the Output button again to turn off the output and the LED.

Note: If there are any of the following conditions, the output will automatically turn off.

- 1. OVP turns on and there are unusual OVP on the output terminal.
- 2. The setting voltage is more than that of the OVP.
- 3. Recalling other setups from the memory.

Beep On / Off

Panel Operation

By default, the beep sound is enabled. To turn off the beep, press the OCP(BEEP) button for 2 seconds. A beep comes out and the beep setting will be turned off. To enable the beep, press the OCP(BEEP) button again for 2 seconds.

Front Panel Lock

Panel operation

Press the LOCK button to lock the front panel button operation. The LED turns on. To unlock, press the LOCK button for 2 seconds.

11