




|                 |                            |                             |
|-----------------|----------------------------|-----------------------------|
| Transformer No. | MED5000                    | 1 -fase / -con. 50 Hz       |
| Customer        | MEDICAL ISOLATION STANDARD | Note                        |
| Assembly Comp.  | CENTER POTTED              | Date/sign. 07-15-2009 KEVIN |

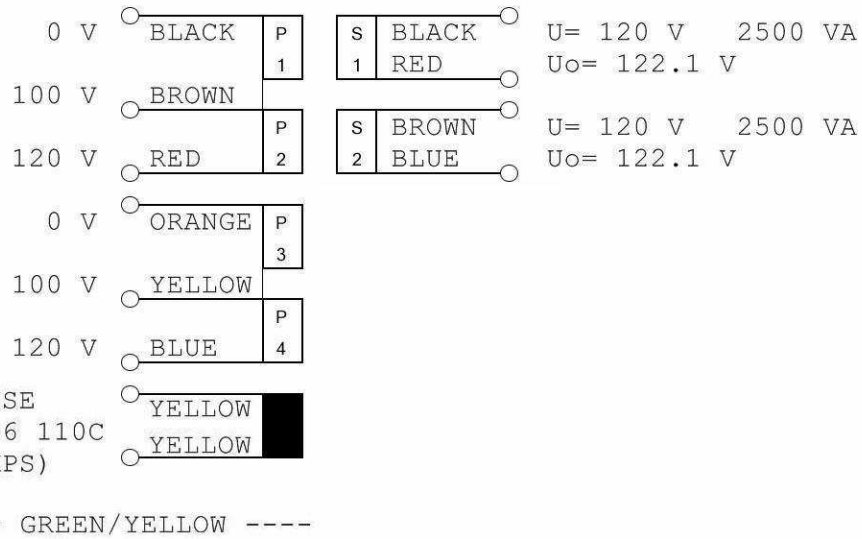

Marking

|   |  |              |
|---|--|--------------|
|  MADE BY AMGIS LLC USA<br>TRANSFORMER P/N MED5000<br>PRIM.2*(0-100-120V) 50/60Hz 5091VA<br>SEC.2*120V 2*2500VA |  | Changed from |
|   |  | Changed to   |
|   |  |              |

|        |                      |                   |                |            |
|--------|----------------------|-------------------|----------------|------------|
| Tests. | Uo. Tolerance, ± 3 % | Iomax: 675.3 (mA) | 100 V over P1. | Isol: 4K V |
|--------|----------------------|-------------------|----------------|------------|

|             |                  |                    |                   |
|-------------|------------------|--------------------|-------------------|
| Dimensions: | Max H: 4.5" (mm) | Max. Ø: 12.3" (mm) | Terminals: 250 mm |
|-------------|------------------|--------------------|-------------------|

|      |   |
|------|---|
| (mm) | Center Potted with 1/2" dia hole                  |
|      | 1 pc neoprene gasket 11" dia x 1/2" ID x 1/4" thk |
|      |   |
|      |   |
|      |   |
|      |   |
|      |   |